

EFFECTS AND CONTROL OF PULSATION IN GAS MEASUREMENT

Class 1090

Ray G. Durke
Senior Research Engineer

Edgar B. Bowles, Jr.
Director – Fluids and Machinery Engineering Department

&

Robert J. McKee, Ph. D.
Retired

Southwest Research Institute
6220 Culebra Road
San Antonio, TX 78238 USA

One of the most common measurement errors and the most difficult to identify in natural gas metering systems is that caused by pulsating flow. It is important to understand the effects that pulsations have on the common types of flow meters used in the gas industry so that potential error-producing mechanisms can be identified and avoided. It is also essential to understand pulsation control techniques for mitigating pulsation effects. This paper describes the effects of pulsation on orifice, turbine, ultrasonic, and other flow meter types. It also presents basic methods for mitigating pulsation effects at meter installations, including a specific procedure for designing acoustic filters that can isolate a flow meter from the source of pulsation.

Pulsation Basics

Pulsation is a periodic fluctuation in local pressure and velocity that occurs throughout a piping system or network. Due to the physics of inviscid fluid flow through a conduit (i.e., the Bernoulli principle), there cannot be a variation in the local pressure (pulsation) without a corresponding variation in the local velocity. Conversely, if velocity perturbations are present, there will be pressure variations, as well, propagating along the pipe. Pulsations travel as acoustic waves, both upstream and downstream from the source. Equation 1 shows the Bernoulli principle (in its simplest form for steady, one-dimensional flow of a compressible fluid (e.g., natural gas) through a conduit) and Figure 1 illustrates the generation of pulsation waves (from a prime mover, such as a reciprocating compressor or pump) and shows how pressure and velocity variations travel in a pipe.

$$\frac{V^2}{2} + \left(\frac{\gamma}{\gamma-1}\right)\frac{P}{\rho} + gz = constant \quad \text{Equation 1}$$

where

- V = nominal fluid velocity
- P = static line pressure
- ρ = fluid density
- g = gravitational acceleration
- z = elevation of a point above a reference plane
- γ = ratio of the specific heats of the fluid

Pulsations typically move through a piping system as traveling waves. These traveling waves can be reflected from 'closed' and 'open' ends of a piping network. 'Closed' ends, for example, may be the capped or flanged ends of headers, closed branch line valves, or terminations of gauge or drain lines. 'Open' ends may not be truly 'open.' For instance, significant and sudden diameter changes, such as at scrubbers, large headers, or locations where a small branch line connects to a larger diameter pipe have acoustic characteristics closely approximating those of a truly 'open' pipe end. Through the principle of superposition, traveling waves can be reflected in a piping network and added together in such a way that summations of the amplitudes of the various waves form peaks (maximums) at some locations and nulls (minimums) at other locations along the pipe network. At certain conditions (characterized by the speed of sound of the flowing medium, the pipe length, and pulsation frequency),

traveling pulsation waves are reflected to form standing waves that reinforce pulsation amplitudes. This condition is known as 'acoustic resonance' and occurs at the natural resonant frequency of the pipe at the given operating conditions.

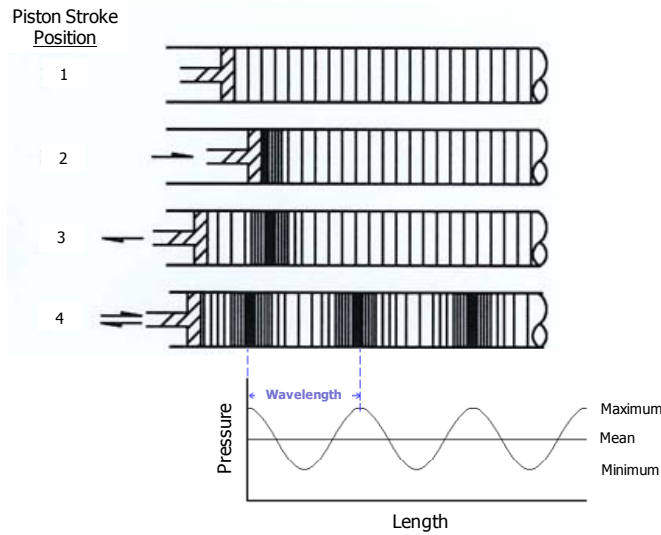


Figure 1. Illustration of Ideal Generation of a Pulsation Wave

The relationship between the speed of sound of the flowing medium, c (a.k.a., the acoustic velocity), the pipe length, L , and pipe end conditions determines the frequency, f , and fundamental wavelength, λ , of the acoustic response. The fundamental wavelength is defined by Equation 2. An acoustic resonance in a piping section is dependent upon the quotient of the speed of sound of the flowing medium, c , divided by the length of the pipe element, L . 'Half-wave' acoustic resonances occur between two open pipe ends or two closed pipe ends. 'Quarter-wave' resonances (i.e., Figure 2) occur between one open and one closed pipe end. Multiples of the fundamental half-wave or quarter-wave resonant modes occur at higher frequencies in the same length of pipe. Simple acoustic theory can be used to estimate the acoustic response frequencies of meter runs, meter headers, and instrument-sensing lines (a.k.a., gauge lines).

$$\lambda = \frac{c}{f} \tag{Equation 2}$$

where

- λ = pulsation wavelength
- c = speed of sound of the flowing gas
- f = pulsation frequency

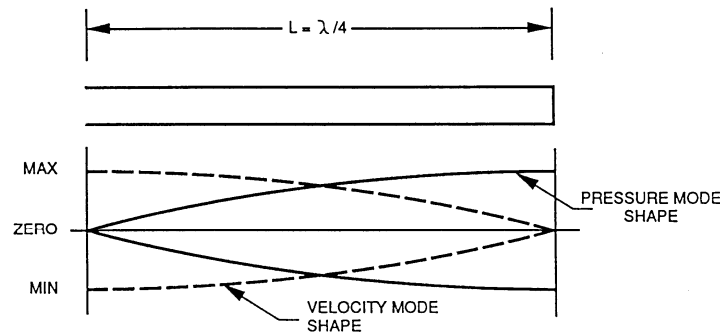


Figure 2. Quarter-wave Pulsation Resonance Between Open and Closed Ends

The amplitude of pulsation in a piping system reaches the largest value during resonant conditions, with pressure maximums in fixed locations and velocity maximums in other, fixed locations. Pulsation problems at flow metering sites frequently involve resonant conditions.

Pulsations in piping systems are created by any flow disturbance or source of periodic pulses or change in the flow rate. Common sources of pulsation in natural gas pipeline systems may include:

- Reciprocating compressors
- Rotary screw or booster compressors
- Centrifugal compressors (away from the optimum design point)
- Pressure regulating or flow control valves
- Rapid load or supply transients
- Vortex shedding and similar flow-induced phenomena
- Fluidic instabilities, such as slug flow

Because compression or pump machinery (and control valves and other unsteady aspects of station operation) are typically in close proximity to flow meter pipe runs, pulsations are common at field sites and can have an adverse effect on flow meter accuracy.

Pulsation Effects on Orifice Flow Meters

Primary Element Error

In the case of orifice flow meters, pulsation affects both the primary flow element (i.e., the orifice plate) and the secondary measurement system (i.e., pressure transducers and the connecting gauge lines). The most basic pulsation-induced error mechanism at an orifice flow meter installation is called square root error (*SRE*) because it results from averaging the differential pressure (ΔP) across a square root response device. Flow through an orifice is proportional to the square root of the differential pressure, ΔP , across the orifice plate, as noted in the simplified orifice flow equation shown in Equation 3. The square root of the *instantaneous* ΔP should be averaged over time for proper flow rate determination. However, typical industrial-grade pressure transducers do not accurately track the rapid pulsating changes in ΔP . Thus, the resulting measurement process captures an *averaged* ΔP reading before the square root value of the ΔP is taken to determine flow rate. This means that *SRE* is inherent in the measurement. Pulsations across the orifice plate must be eliminated to avoid *SRE* being introduced when *average* ΔP s are recorded by the measurement system. Figure 3 shows the relationship between ΔP and flow rate for an orifice and indicates what happens when pulsating flow exists.

$$\Delta P = K * Q^2 \qquad \text{Equation 3}$$

where

ΔP = differential pressure measured across the orifice plate

K = empirical coefficient

Q = volumetric flow rate

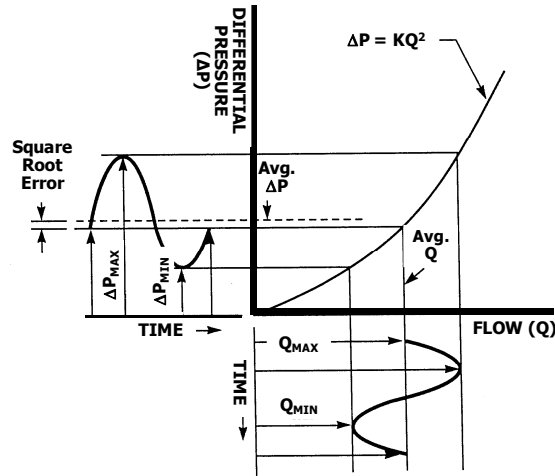


Figure 3. Square Root Error Results from Pulsation Effect on an Orifice's Square Law Curve

As seen in Figure 3, the average ΔP signal is slightly higher than the ΔP that corresponds to the average flow. The square law relation between flow rate, Q , and the differential pressure across the orifice plate, ΔP , creates this distortion through the square law curve, since a larger portion of the ΔP wave occurs above the average flow line. Therefore, when the ΔP signal is averaged by a measurement-grade ΔP transmitter, the average ΔP is higher than the ΔP that corresponds to the average flow. This real difference in ΔP across the orifice plate is the pulsation effect known as *SRE*.

SRE is always positive and increases with increasing pulsation amplitude. *SRE* is a data processing error resulting from averaging the ΔP signal before taking its square root. This usually cannot be avoided when industrial-grade pressure transmitters are used because transmitters of this type have a relatively low operational frequency range, which prevents the transmitters from accurately tracking the rapidly-varying pressure signals produced by flow pulsations; hence, they provide an 'averaged' value instead. Furthermore, digital or 'smart' pressure transmitters take a small, but finite, amount of time to record and transmit the measured pressure values for processing by data logging devices, such as flow computers or supervisory control and data acquisition (SCADA) systems. A consequence of this whole data acquisition process is that the differential pressure across the orifice plate is usually averaged over some finite period of time before the square root of the resultant value is calculated, thus, creating the *SRE*.

If one uses a pressure transmitter with a frequency response range high enough to accurately measure the differential pressure across an orifice plate experiencing pulsating flow, the mathematical relationship shown in Equation 4 can be utilized to determine the magnitude of the *SRE*. This method for determining *SRE* is a patented process developed at Southwest Research Institute during research sponsored by the Gas Machinery Research Council and is the basis for the commercially-available Square Root Error Indicator that measures the *SRE*.

$$SRE = \frac{\sqrt{avg\Delta P} - avg\sqrt{\Delta P}}{avg\sqrt{\Delta P}} * 100 \quad \text{Equation 4}$$

where

- SRE = the square root error in percent of differential pressure transmitter reading
- $\sqrt{avg\Delta P}$ = the square root of the time averaged value of the differential pressure across the orifice plate
- $avg\sqrt{\Delta P}$ = the time averaged value of the square root of the instantaneous differential pressure across the orifice plate

SRE usually accounts for most, but not necessarily all of the pulsation-induced error associated with an orifice flow meter. Inertial effects can also contribute to measurement error. Inertial effects typically don't become problematic unless relatively high-amplitude pulsations occur at relatively high frequencies. Because *SRE* usually develops well before inertial effects become significant, inertial effects are generally ignored when diagnosing the adverse effects of pulsation.

Error due to inertial effects can be derived from the one-dimensional momentum equation for steady flow through an orifice. The momentum equation for unsteady flow may also be used to develop the orifice flow equation, but a time rate of change term must be included also. In Equation 5 below, the term to the right represents the fluid inertia term, which includes the derivative of the fluid velocity with respect to time and accounts for the extra differential pressure needed to accelerate or decelerate the gas as it flows through the orifice. One feature of the inertial effect is that when it is averaged over time, the average is *zero*. However, if the square root of the instantaneous differential pressure, ΔP , across the orifice is recorded correctly to eliminate *SRE*, then the inertia effect is *not zero*.

$$\Delta P = K * V(t)^2 + L \frac{dv(t)}{dt} \quad \text{Equation 5}$$

where

- ΔP = differential pressure across the orifice plate
- V = nominal gas velocity
- L = pulsation wave acoustic length
- K = proportionality constant
- t = time

It is important to note that the measured amount of *SRE* cannot be used to perfectly correct for orifice measurement error associated with flow pulsation, but *SRE* can be used to indicate if pulsation is causing a significant problem at an orifice flow meter. The maximum allowable pulsation level specified in Section 2.6.4 of Part 2 of American Gas Association (AGA) Report No. 3, i.e., the U.S. orifice flow meter standard, is 10% root mean square (RMS) variation in the ΔP (RMS is a statistical measure of the magnitude of the variation in the ΔP), which corresponds to an *SRE* value of approximately 0.125% of reading. This applies to single frequency flow pulsations with or without several harmonics and to broad-band flow pulsations/noise. Any *SRE* above this threshold indicates that the pulsation is adversely affecting the orifice meter accuracy. Section 2.6.4 further states that... *“Currently, no satisfactory theoretical or empirical adjustment for orifice measurement in pulsating flow applications exists that, when applied to custody transfer measurement, will maintain the measurement accuracy predicted by this standard. Arbitrary application of any correcting formula is may even increase the flow measurement error under pulsating flow conditions. The user should make every practical effort to eliminate pulsations at the source to avoid increased uncertainty in measurements.”*

Secondary Element Error

Pulsation may also adversely affect the secondary measurement system (i.e., the gauge lines connecting the pressure transmitters to the meter fitting and the pressure transmitters themselves) of an orifice meter installation. The gauge lines that connect the pressure transmitters to an orifice fitting can *amplify* the pulsation amplitude or *attenuate* the pulsation amplitude and, in the process, change the apparent ΔP value. When gauge line *amplification* occurs, as shown in Figure 4, the actual pulsation amplitude in the pipe and *SRE* at the orifice meter might be small and the effect of pulsation on the orifice flow measurement should be negligible. However, pulsation at the differential pressure transmitter appears high and if *SRE* is occurring at the end of the gauge lines, an apparent (and significant) pulsation error results. Gauge line amplification is usually a result of a gauge line being by pulsation at its fundamental acoustic frequency (i.e., 100 Hz in the example shown in Figure 5) or one of its higher orders. Figure 5 illustrates the frequency response characteristics of an example gauge line (illustrating both pressure signal *amplification* and *attenuation* effects, depending on the frequency). It is desirable for the pressure measured at the transmitter, P_t , to be exactly equal to the pressure at the orifice, P_o (i.e., $P_t/P_o=1.0$, as shown in Figure 5). It is critically important to also note that the measurement systems used to determine *SRE* are also subject to pulsation amplification and care should always be taken to ensure that real pulsations across the orifice pressure taps are not amplified in the gauge lines to the pressure transmitter being used to detect the presence of *SRE* at the orifice meter.

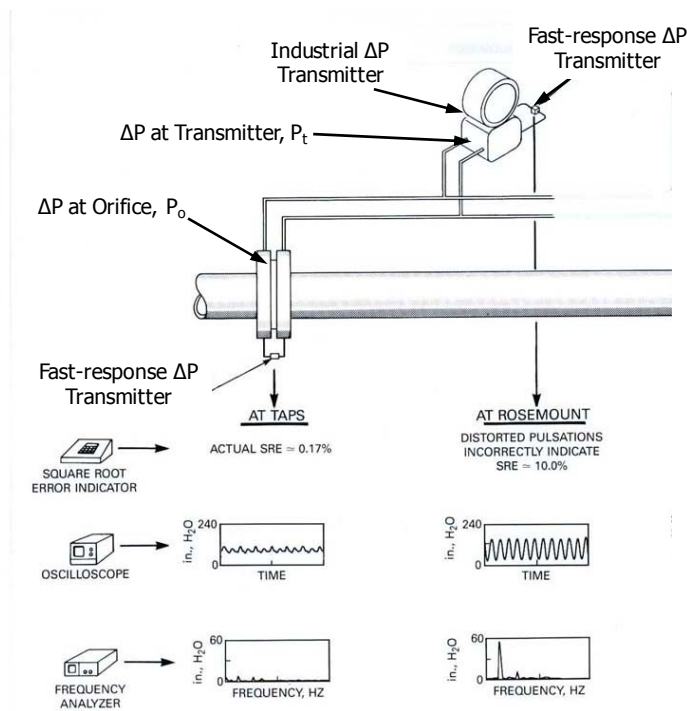


Figure 4. Amplification of Orifice Meter Differential Pressure Signal in the ΔP Transmitter Gauge Lines

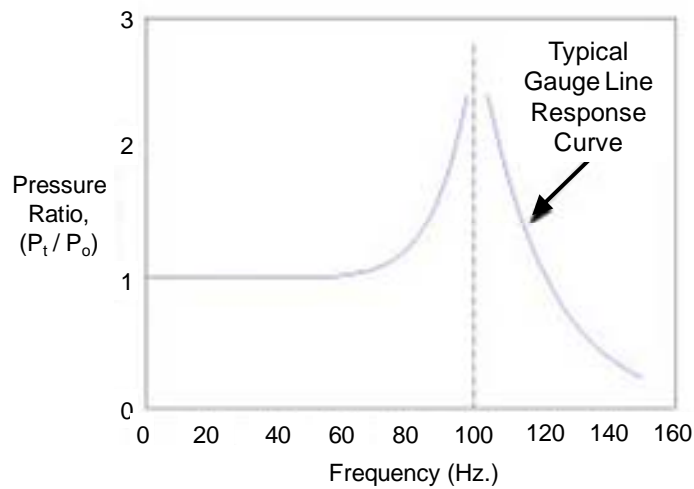


Figure 5. Example Frequency Response Characteristics of a Constant-bore Gauge Line

Gauge line *attenuation*, which can occur when gauge lines are not responsive to the pulsation frequency, has the opposite effect as amplification. When attenuation occurs, there can be large pulsation amplitudes and a significant *SRE* at the orifice meter, while there is little or no indication of pulsation at the ends of the gauge lines connected to the differential pressure transmitter. If attenuation is present and *SRE* is measured at the end of the gauge line, then a pulsation error can be missed.

Experience has shown that the likelihood of gauge line effects becoming a problem can usually be reduced or avoided by minimizing the lengths of all gauge lines (since the acoustic natural frequency of a gauge line is inversely proportional to line length) or by mismatching the acoustic response of the gauge lines with respect to the meter tube pulsation frequencies. For example, close-coupling the pressure transmitter(s) (and associated valving) to a sensor orifice fitting, as shown in Figure 6, can increase the response frequency of the gauge lines, such that when a low-speed compressor is the pulsation source, the pulsation excitation frequency is mismatched with respect to the acoustic response of the gauge lines. This close-coupled configuration may still be

problematic when a high-speed compressor is the pulsation source. In that instance, the lower pulsation harmonic frequencies (e.g., fourth-order of compressor running speed) may coincide with the acoustic response of the gauge lines, thus, producing in gauge line error.

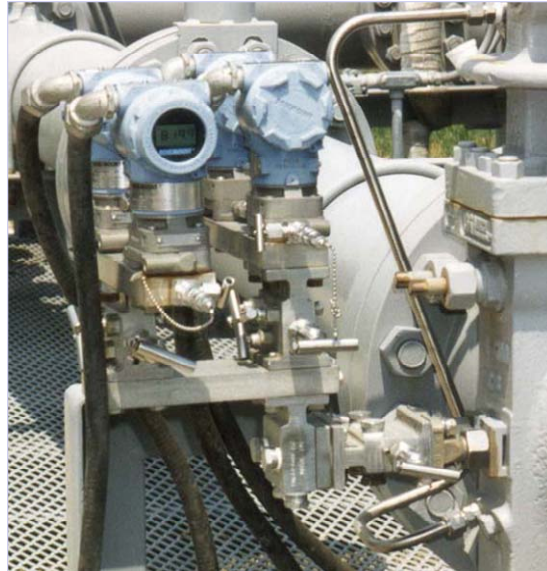


Figure 6. Example Close-coupled Pressure Transmitter Installation
(recommended to minimize the likelihood of gauge line effects)
(Image provided courtesy of PGI International, Inc.)

Gauge line *shift* is a change in ΔP along the length of a gauge line and is a result of phenomena associated with the gas alternately flowing into and out of a gauge line. Example results from laboratory measurements at Southwest Research Institute of pressure along a gauge line with pulsation present are shown in Figure 7. There is a change in the pressure at the entrance to the gauge line (i.e., at the orifice meter pressure taps) and there is a pressure gradient along the gauge line. One reason for these changes in gauge line pressure under dynamic conditions is that the resistance to flow into the gauge line is less than the resistance to flow out of the gauge line. Frequency-dependent influences can also contribute to gauge line shifts. Research has shown that the amplitude of a gauge line shift is related to the velocity head and is usually only on the order of a few inches of water column differential pressure. Gauge line shift does not usually make a significant difference in static pipeline pressure measurements. However, a few inches of water column difference out of perhaps 30 to 50 inches of water column total differential pressure across an orifice plate can result in a relatively large flow measurement error.

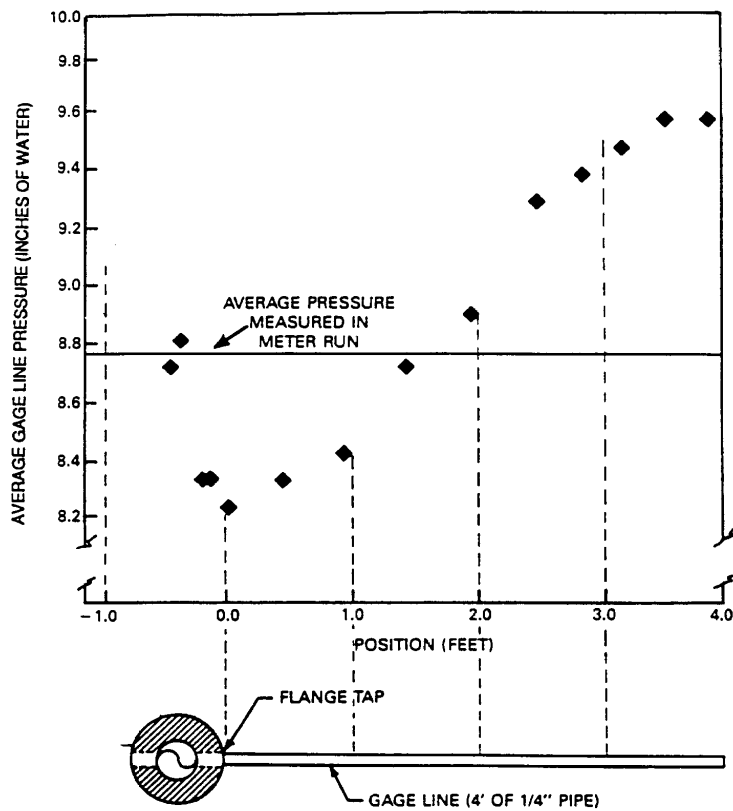


Figure 7. Measured Pressure Along a Gauge Line Indicating a Shift in Differential Pressure

To correctly sample gas pressure in pulsating flow, a pressure transmitter must be capable of accurately sampling and recording the pressure signal at a frequency of at least twice (and, preferably, 10 times) the highest pulsation frequency present in the flow. Sampling and recording a transmitter output at a frequency slower than at least two times the maximum pulsation frequency will cause data describing actual flow changes to be lost and flow measurement error will result. It is important to note that industrial-grade analog and digital (i.e., 'smart') pressure transmitters used today by the natural gas pipeline industry, are not capable of sampling at a high enough frequency to precisely follow the typical variation in pressure caused by pulsations. This point is illustrated in Figure 8, which demonstrates the responsiveness of industrial-grade pressure transmitters, typical of those used at gas meter stations, to a sudden change in pressure. A test was set up in which each pressure transmitter was initially exposed to its maximum rated working pressure (denoted in Figure 8 as a transmitter output of 20 milliamps – the maximum output signal for a transmitter having a 4 to 20 milliamp output range). The test pressure was suddenly dropped to zero gauge pressure (i.e., atmospheric pressure) and the response of each transmitter was recorded. The time required for the test pressure to drop to its minimum value (i.e., 4 milliamps transmitter output value) was less than 0.1 second. The outputs of some of the transmitters took well over one second to reach the minimum test pressure. Clearly, pressure transmitters of this type are not able to accurately measure typical pulsation pressure fluctuations occurring at frequencies of one cycle per second and higher.

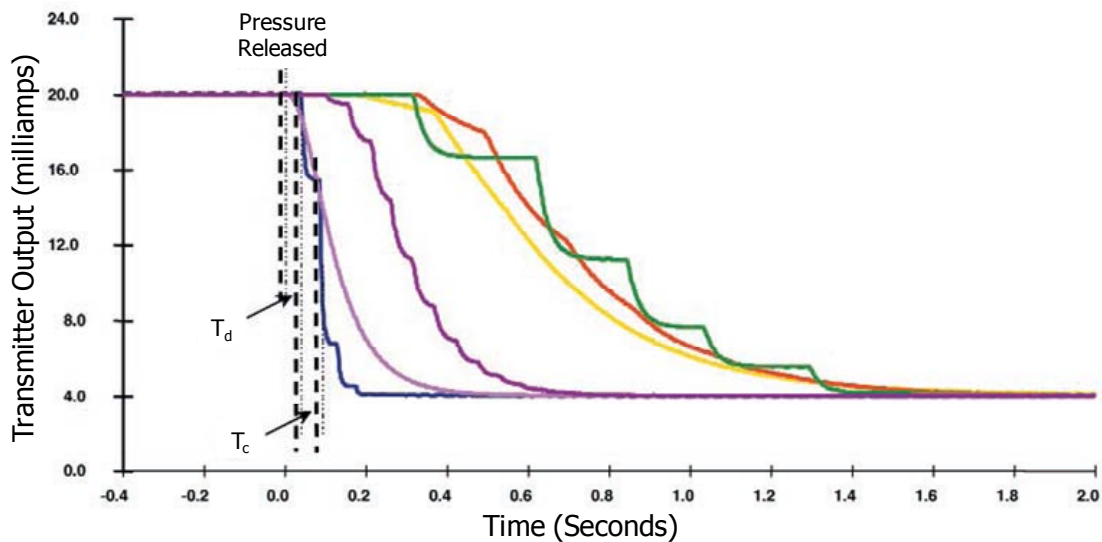


Figure 8. Industrial Pressure Transmitter Response to Test Pressure Step Change
 (Source: Rosemount, Inc., *Pipeline and Gas Journal* article, published in 2001)

Square Root Error Indicator

In order to diagnose properly any *SRE* that may exist at an orifice flow meter, 'fast-response' pressure transmitters capable of accurately measuring the pressure variations associated with pulsating flow should be used. The *SRE* Indicator described previously has been purpose built for such applications. The latest version of the *SRE* Indicator (distributed by PGI International, Inc.) is pictured in Figure 9. An example *SRE* analysis produced by the *SRE* Indicator is pictured in the computer screen capture shown in Figure 10. The example analysis shows the existence of a high-frequency pulsation (at a frequency of about 163 Hz) superimposed over the differential pressure being measured across an orifice flow meter. As the screen capture notes, the estimated *SRE* in this example is approximately 0.468% of the measured flow rate.

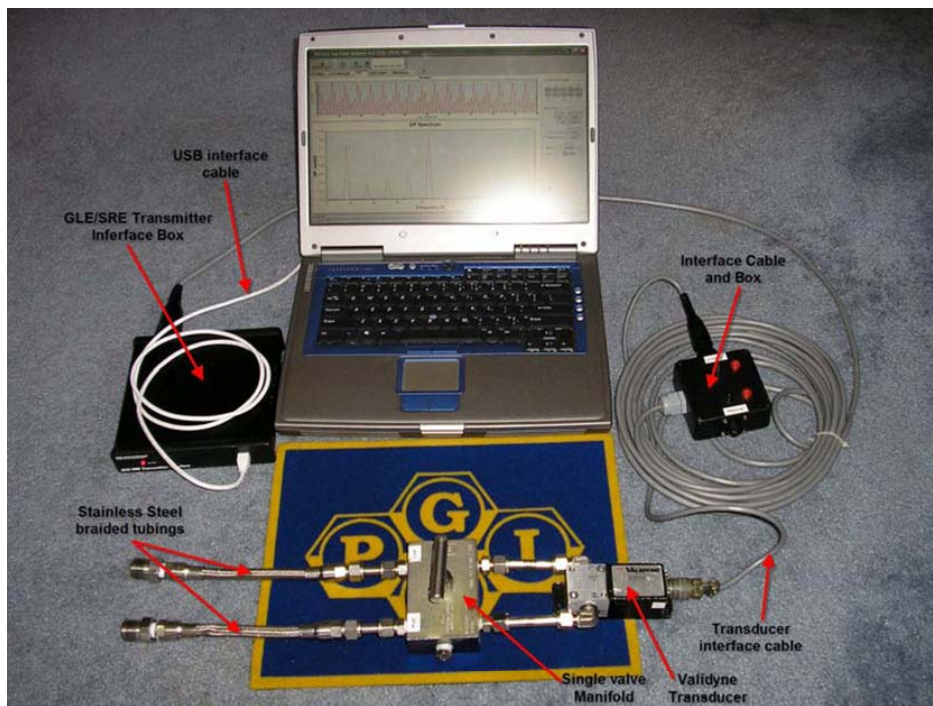


Figure 9. Square Root Error Indicator
 (Image provided courtesy of PGI International, Inc.)

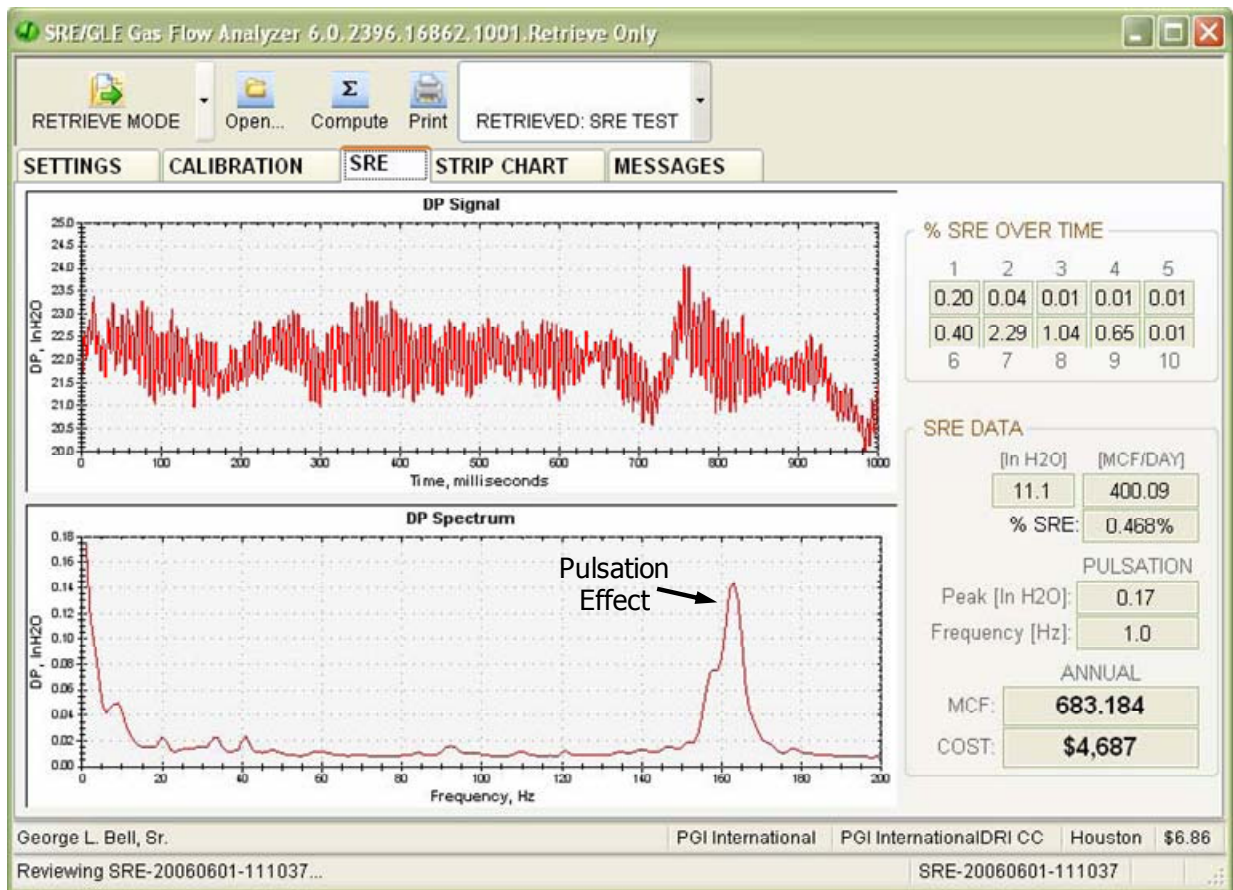


Figure 10. Example Analysis Produced by the Square Root Error Indicator
(Image provided courtesy of PGI International, Inc.)

Pulsation Effects on Turbine Flow Meters

Turbine flow meters can be adversely affected by pulsation, which can cause flow rate measurement errors as large as 50% of meter reading, depending on many factors, including the pulsation velocity amplitude at the meter, flow rate, gas density, and both meter and pulsation properties. The effects of pulsation on turbine meters are somewhat complex but when an error exists, it almost always results in an over-registration, compared to the actual or 'true' flow rate. In recognition, AGA Report No. 7 (i.e., the U.S. natural gas industry recommended practice for turbine flow meters) notes that pulsation causes a positive error in turbine meter output that is dependent upon the factors listed above. AGA Report No. 7 also recommends that in order to avoid pulsation-related measurement errors, pulsation should be eliminated by filtering or reduced by taking a pressure drop to dampen the pulsation.

A number of flow tests have been conducted with turbine meters in pulsating flow. Example results produced at the Southwest Research Institute flow laboratory are shown in Figure 11, where the zero error 'baseline' or reference flow rate value is for the flow meter output recorded with a steady flow condition, free of any pulsations. The pulsation-induced flow measurement errors in this test varied from zero to over 20% of meter reading, depending on the flow rate and the pulsation frequency. Pulsation amplitudes were essentially identical for all flow tests. The observed frequency dependence was due to the pulsation mode shape and resulting velocity modulation changing at the flow meter location, which was at a fixed point in the flow facility piping network. Turbine meters are velocity-measuring devices and, as such, are more sensitive to gas velocity variations than to gas pressure variations. At some pulsation frequencies, the velocity modulation at the meter will be large and the flow measurement error will be large, while at other frequencies, the velocity modulation at the meter and corresponding measurement error will be small, despite the overall pulsation level being relatively high. Pulsation effects at a turbine meter can be mitigated by reducing the pulsation amplitude or by changing the meter location with respect to the pulsation mode shape, such that the velocity modulation at the measurement point is relatively low.

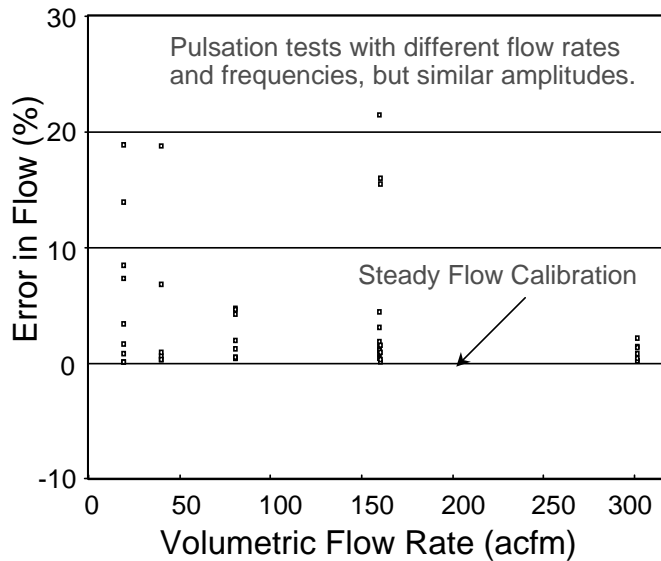


Figure 11. Example Pulsation Test Results for a Turbine Flow Meter

Pulsation Effects on Ultrasonic Flow Meters

As with other metering technologies, ultrasonic flow meters can be adversely affected by pulsation. Ultrasonic meters that measure high-pressure natural gas flows typically use a time-of-flight (or transit time) measurement technique. Figure 12 shows a typical design configuration. A high-frequency (i.e., >100,000 Hz) acoustic pulse (or pressure wave) is broadcast through the flow field from a sending transducer (shown as 'A' on Figure 12). The pulse travels at an acute angle across the pipe to a receiving transducer (shown as 'B' on Figure 12). The receiver may be located on either the opposite side or the same side of the pipe as the sending transducer. If the sending and receiving transducers are on the same side of the pipe, the acoustic beam is reflected off the opposite pipe wall before being received. Ultrasonic energy pulses are sent in both the 'upstream' and 'downstream' direction across one or more acoustic paths that traverse the pipe. The differences in these transit times provide an indication of the flow velocity in the pipe, which can be correlated to the volumetric flow rate. The measured times are affected by several factors, including the velocity profile of the gas stream at the measurement point and the acoustic signal characteristics, among others. The ultrasonic pulses are typically sent through the flow stream many times per second. The meter electronics process the measured data and average the results before outputting a flow rate value approximately once to several times per second. Because the method used is inherently sampling the flow periodically, instead of continuously, meters of this type may not perfectly track the rapid changes in the flow field that can occur during pulsating flow. Hence, measurement errors can result.

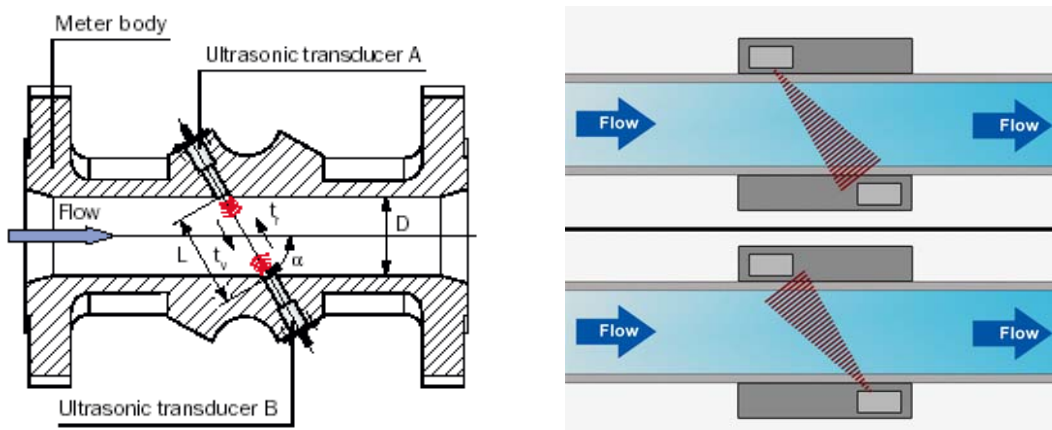


Figure 12. Schematic of an Ultrasonic Flow Meter
(Images courtesy of Bureau of Analytical Complexities & Systems and Alicat Scientific)

There is a limited amount of test data on the effects of pulsations on ultrasonic flow meter accuracy. Ultrasonic flow meter error does not appear to closely correlate to the amplitude of the pulsation *pressure*. The flow rate measurement generally depends on the pulsation *velocity* amplitude, and errors as great as several percent of meter reading (or even greater, in some instances) have been reported in the open literature (see Figure 13, for example). Errors of over-registration relative to the 'actual' or 'true' flow rate, as well as errors of under-registration have been reported. Reported causes of errors associated with pulsations include:

- Aliasing of the measured flow values due to inadequate flow data sampling frequency by the meter. However, at least some test results have shown that higher data sampling rates do not necessarily reduce the magnitude of the measurement error.
- Velocity profile variations or distortions due to pulsation effects.
- Location of the meter relative to node points when standing pulsation waves exist (i.e., node points are points along the flow stream where the velocity is unchanging even though pulsations are present). Meter error is a function of the local velocity modulation amplitude when standing pulsation waves exist.

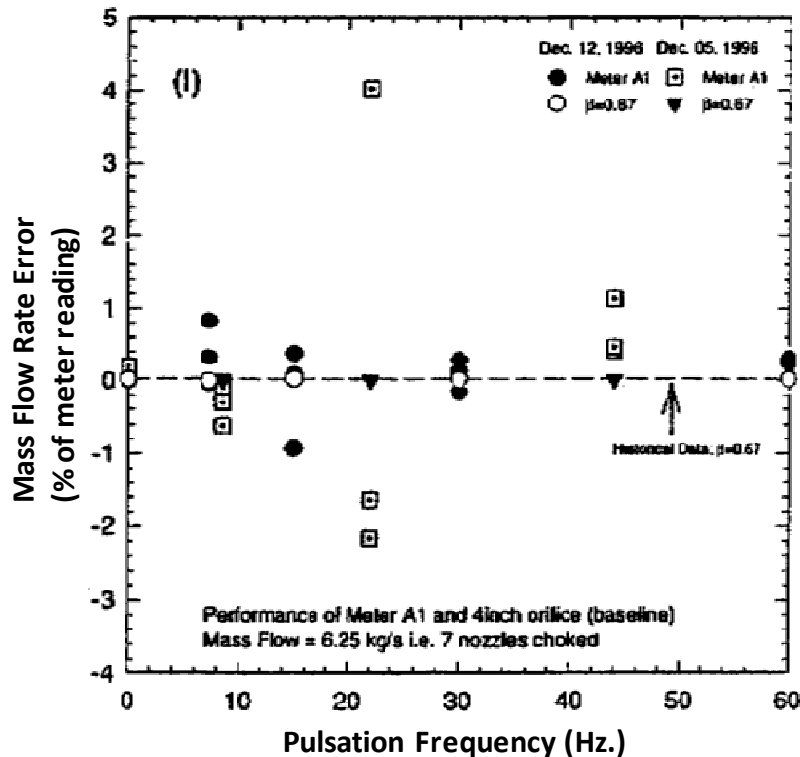


Figure 13. Example Pulsation Effects on Ultrasonic Flow Meter Accuracy

(Source: NOVA Research and Technology Centre, *International Pipeline Conference* paper, published in 1998)

Ultrasonic meters may also be affected by pulsation from broadband ultrasonic noise sources, such as pressure regulating valves, which may produce background acoustic noise in the flow stream that could potentially interfere with the acoustic pulses produced by the flow meter. In these cases, the usual solutions are to either greatly reduce or eliminate the pulsation and background acoustic noise present at the flow meter or to change the operational frequency range of the meter transducers.

Other Flow Meters

Most other gas flow meter types, including Coriolis flow meters, Pitot probes, multi-port Pitot probes, V-cone flow meters, Venturi flow meters, and vortex shedding flow meters, can also be adversely affected by the presence of pulsation in the flow stream. The differential producing meters in this group are affected in ways similar to those for the orifice flow meter.

Coriolis meters, which sense the vibratory motion of fluid-containing tubes, are generally affected by vibrations caused by pulsation and can be severely affected at some pulsation frequencies and less affected at other frequencies.

Pitot probes and the multi-port Pitot probes typically have a dynamic response similar to that of pressure transmitter gauge lines and, therefore, can be adversely affected by pulsation. Some frequency-specific adjustments can be made to particular meters, such as vortex shedding meters, to correct for some types of pulsating flow conditions, but this is not usually a correction that is effective when a range of pulsation conditions may exist at a particular meter installation.

Several types of positive displacement meters, including diaphragm meters, are generally insensitive to pulsation effects, but these meter types are not very useful for high-volume flows. Rotary-type positive displacement meters, for example, are not normally subject to errors in pulsating flow but they do produce pulsations because of the nature of their design and can, therefore, adversely affect parallel or nearby flow meters of other types. In general, the best approach to eliminating metering errors in pulsating flow is to mitigate the pulsation levels.

Pulsation Control Methods

Several approaches for mitigating pulsation effects in gas flow measurement are available. The most practical method for a particular situation will depend on the meter type and the pulsation characteristics. The most effective method for mitigating pulsation effects is installation of an acoustic filter. Acoustic filters are less dependent on the source of pulsation or the type of meter than other mitigation approaches because acoustic filters isolate a flow meter from pulsation sources. There are multiple configurations to consider when designing acoustic filters, so it is advisable to consult an experienced designer when considering installation of an acoustic filter. Following shortly is an example design of a symmetric, in-line, low-pass acoustic filter that works well in many pulsation isolation situations.

There are other techniques for mitigating pulsation effects for particular pulsation sources, selected meter types, or situations where only a small improvement is needed. For instance, a large pressure drop can be taken when a less costly, although less effective, approach is required. It is noteworthy that separating a flow meter from a pulsation source by a significant distance is *not* usually an effective pulsation mitigation strategy because pulsations can travel great distances. For instance, low-frequency pipe flow pulsation (e.g., a 2 Hz pulsation) can have an adverse effect on a flow meter located over 20 miles from the pulsation source. Typical pipeline pulsation frequencies in the 5 to 45 Hz range can propagate several miles from the source and higher frequencies (e.g., over 100 Hz) can exist at significant levels hundreds of yards to a mile from the source. Thus, placing a meter at a location well removed from a pulsation source is not usually effective (or practical) for mitigating pulsation effects. In select cases, relocating a meter a considerable distance from a pressure regulator or a flow control valve that is producing primarily high-frequency noise may prove effective.

If standing wave pulsations exist, then placement of a flow meter relative to the local standing wave pattern can be important. For example, if the acoustic wave characteristics of a particular meter installation are known, it may be possible to place, say, a turbine meter at a point in the pipe network where the pulsation mode shape produces a negligibly small velocity modulation for all operating conditions. In that instance, the pulsation effect on the flow meter may be minimal or nonexistent. The center point of a flow meter run between two large-diameter headers (open ends) is a location with negligible velocity modulation for the first-order, half-wave resonance.

Selecting pipe lengths to avoid acoustic resonant frequencies can be an effective mitigation technique when a specific pulsation frequency or acoustic wave mode shape is a problem. For instance, if a nearby compressor is to operate at a fixed running speed, the flow meter run and header lengths should *not* be designed as half-wavelengths or quarter-wavelengths for that particular driving frequency. Meter runs, headers, and pipe segment lengths should *not* be simple fractions of the speed of sound of the flowing medium divided by the compressor running speed (in Hertz). In a case in which the compressor speed varies significantly, there may not be an acceptable pipe length that can avoid all potential pulsation problems.

A change of pipe length can be very effective in the case of a side-branch pipeline that is excited by vortex shedding created by the flow through the pipe. Changing the branch line length can prevent the resonance and significantly reduce the pulsation amplitude. For orifice flow meters, the pressure transducer gauge line length should be selected to avoid resonance at compressor running speed or other known excitation frequencies. A change in pipe length can be considered for any resonance pipe if the change will eliminate pulsation rather than just change the pulsation frequency.

Addition of pressure drop via installation of an orifice (or restricting valve) can produce a reduction in pulsation amplitude, but it will not eliminate a pulsation or change its frequency. However, in most cases, additional pressure drop is not practical. Furthermore, achieving an effective solution by adding an orifice may end up being a trial-and-error approach, unless a detailed acoustic analysis of the situation is part of the process.

One pulsation mitigation technique that applies specifically to orifice flow meters is the reduction of the orifice beta ratio, which, in turn, increases the ΔP . As long as the pulsation amplitude remains constant, the *SRE* effect on the orifice will be reduced. In many cases, changing the orifice beta ratio will not affect the amplitude of pulsation.

A final comment on pulsation mitigation methods is that large vessels are not acoustic filters and will not necessarily eliminate or completely remove pulsation but, in many cases, may attenuate or absorb some pulsation amplitude. Scrubber vessels and large headers can be placed strategically and may be utilized to help reduce pulsation amplitudes.

Acoustic Filter Design

The most effective method for controlling pulsation in metering applications is to place an acoustic filter between the pulsation source and the flow meter to be protected. There are many approaches to designing acoustic filters. The filter design described below and pictured in Figure 14 is a symmetric, in-line, low-pass acoustic filter that performs can be used in many situations to eliminate pulsation in selected frequency ranges. As the name implies, this filter passes pulsation below its natural frequency and filters out (or, at least, significantly reduces) pulsation at frequencies above the natural frequency. One important characteristic of this type of filter is that it amplifies pulsation at and near its natural frequency. Therefore, pulsation energy that is to be controlled should never be coincident with the natural frequency of the filter. Filters of this type are placed directly in the mainline pipe and are symmetric, meaning that the acoustic length of each element, i.e., a volume, a choke, and another volume, is the same. Other acoustic filter types can be non-symmetric, take up less space, be used on side branches, and have special characteristics when properly designed.

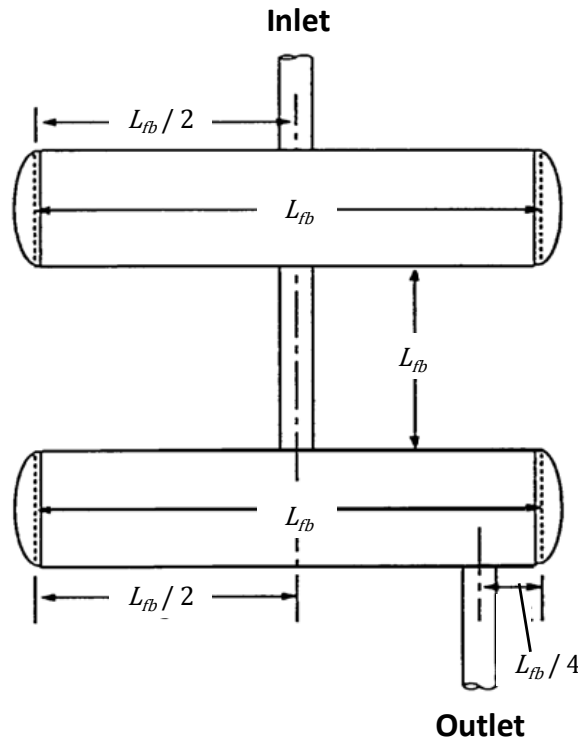


Figure 14. Example Symmetric, In-line Acoustic Filter Design

Operating conditions, such as gas stream pressure, temperature, composition, flow rate, and pulsation frequency of interest, must be known before an in-line acoustic filter can be designed. The following steps and simplified equations can be used to size a symmetric volume–choke–volume filter for typical natural gas pipeline meter station applications.

The first step involves calculating the natural frequency of the filter, which should be at least 20 to 40% below the lowest expected pulsation frequency. The lower this frequency, the larger, and more costly, the acoustic filter.

The second step is to determine the choke tube size. The choke tube internal velocity is selected to be approximately 100 feet per second at the highest expected flow rate. Slightly higher choke tube velocities can be used to reduce the filter size, if a higher system pressure drop can be tolerated. A lower choke tube velocity can be used to reduce pressure drop. However, that will result in a larger and more costly filter. A bell mouth can be added to the choke tube inlet to reduce pressure drop without any adverse effect on the acoustic performance of the system. With a known volumetric flow rate, Q (in cubic feet per second), the following equation, Equation 6, gives the first estimate of choke tube inside diameter. The actual inside diameter of the choke tube, ID_{ct} , selected should be the closest standard pipe size of heavy wall pipe that is larger than the calculated inside diameter. Heavy wall pipes are used in this example and are typically acceptable for gas pipeline applications, but dynamic forces from pulsation act on the filter elements and need to be considered in the design and specification of the system components.

$$ID_{ct} = 1.354\sqrt{Q} \quad \text{Equation 6}$$

After the choke tube size is determined, the third step is to calculate the inside diameter of the pulsation filter bottles, ID_{fb} , which must be at least four times larger than the choke tube diameter in order to be acoustically effective. It is practical, however, to choose a filter bottle diameter that is 8 to 12 times larger than the choke tube diameter so that the filter length will not be excessive. Select a practical first guess for the filter bottle inside diameter that has a heavy wall thickness. After selecting an available inside diameter, the acoustic length, L_{fb} , for filter elements can be calculated from Equation 7.

$$L_{fb} = \frac{0.225 * c * ID_{ct}}{f_o * ID_{fb}} \quad \text{Equation 7}$$

where c is the speed of sound of the flowing gas and f_o is the planned natural frequency of the filter. If this length is unreasonable or uneconomical, then a different inside diameter for the filter bottle can be selected, as long as it is at least four times larger than the inside diameter of the choke tube.

For symmetric acoustic filters, all of the elements have the same effective acoustic length. One geometric adjustment required due to end effects is that the choke tube should be shortened by 1.2 times its inside diameter. The filter bottles need to have a seam-to-seam length that gives them the same inside volume as their cross sectional area times the calculated acoustic length. Accounting for dished heads on the bottle end caps, this gives a seam-to-seam length that is shortened by the bottle diameter divided by six plus two inches for the skirt of the head on each end of the bottle. The result is that the internal volume with the heads included is the same as the acoustic length times the cross sectional area. Then, the filter elements can be assembled as a volume–choke–volume filter, as shown in Figure 14.

The filter inlet pipe enters the acoustic center of the first filter volume. The filter outlet pipe comes off at the 1/4 acoustic length point from the second bottle. If this arrangement is not used, then selected pulsation frequencies, called pass-band frequencies, can propagate through the filter. The choke tube connects the centers of the two acoustic filter bottles. The main lines entering the filter bottles (sometimes referred to as nozzles) can be the same diameter as the mainline piping, which is usually larger than the choke tube diameter and much smaller than the filter bottle diameter. The pipe connections to the filter bottles should be reinforced with saddles or pads. Weld-o-lets should not be used for the connections because of the high local stresses created by weld-o-lets.

As an example calculation, consider the case of a reciprocating compressor nearby a meter station and operating between 300 and 360 RPM. The compressor is always double-acting and is affecting a flow meter run located approximately 200 feet from the suction of the compressor. Double-acting compressors tend to cancel or significantly reduce the amplitude of their fundamental pulsation frequency and show higher pulsation amplitudes at the second and fourth orders of compressor running speed. For this example, the fundamental pulsation frequency ranges for 5 to 6 Hz and the second order ranges from 10 to 12 Hz. The second order pulsations need to be filtered out, but the natural frequency of the filter should also not coincide with the fundamental pulsation frequency. In this case, the natural frequency of the filter can be placed at 8 Hz, which is between the second compressor orders and 20% below the main pulsation frequency to be eliminated (i.e., 10 to 12 Hz).

The flow rate in this example is assumed to be 10.5 MMSCFD at a pressure of 925 psia and a temperature of 75°F. Specific gravity of the gas is assumed to be 0.61. The volumetric flow rate is found to be 2.038 cubic feet

per second and the speed of sound of the gas is calculated as 1,416 feet per second. Equation 6 is used to calculate the choke tube inside diameter, which is determined to be 1.933 inches. The selected choke tube inside diameter is 1.939 inches (i.e., the inside diameter of heavy-wall, two-inch diameter steel pipe). The filter bottle inside diameter needs to be at least 7.75 inches, but to avoid an awkward layout, an inside diameter of 13.124 inches is selected instead. This is the inside diameter of heavy-wall, 14-inch diameter steel pipe. With this diameter, the acoustic element length is calculated from the length equation, Equation 7, to be 5.888 feet. Because of end effects, the physical length of the choke tube should be 5.694 feet.

Conclusions

Pulsating flow, that is, the periodic variation in flow velocity and pressure, can adversely affect flow measurement devices. Flow meter types vary and the error mechanism(s) for each can differ. Some, such as the orifice flow meter, are sensitive to ΔP pulsation amplitudes, while others, such as the turbine flow meter, are sensitive to velocity modulation amplitude and frequency content. Diagnosing pulsation-induced measurement error requires knowledge of the error-producing mechanism(s) and, often, special diagnostic instrumentation and testing techniques.

One of the most reliable ways to avoid flow measurement errors related to pulsating or unsteady flow is to minimize or, preferably, eliminate pulsations at the flow meter. Unfortunately, pulsations can be generated by a number of pipeline sources ranging from reciprocating compressors, flow past piping branch connections, and flow stream blockages, such as valves, pressure regulators, and thermowells. Once created, pulsations can be amplified by acoustic responses throughout the piping system. As demonstrated in this paper, a properly designed low-pass acoustic filter offers a reliable means to attenuate pulsations past the filter.

References

American Gas Association Report No. 3, "Orifice Metering of Natural Gas and Other Related Hydrocarbon Fluids," Part 2, "Specification and Installation Requirements," Washington, D.C., Fourth Edition, April 2000, Second Printing, June 2003.

Sparks, C. R. and John P. Harrell, Jr., "Technical Note - Square Root Error Indicator Gage Line Effects," Gas Machinery Research Council, Southwest Research Institute, San Antonio, TX, April 1996.

Karnik, U., W. Studzinski, J. Geerligs, and M. Rogi, "Effect of Flow Conditioners and Pulsation on the Performance of 8-inch Multi-path Ultrasonic Flow Meters," International Pipeline Conference, Calgary, Alberta, Canada, ASME IPC Paper No. 98-082, June 9-14, 1998.